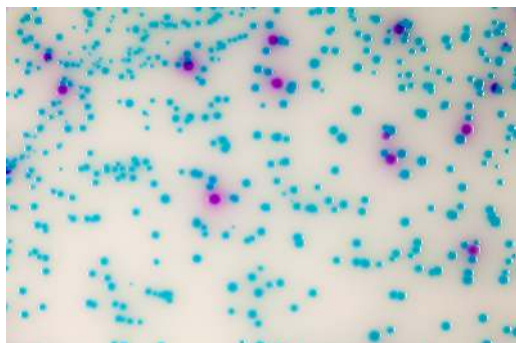


**INSTRUCTIONS FOR USE**
**ChromArt**
**CHROMOGENIC SALMONELLA AGAR**
**Ready-to-use plates**

 CSA: *Salmonella* colonies (magenta-red) and *E. aerogenes* colonies (blue-green)

**1-INTENDED USE**
*In vitro* diagnostic. Selective and chromogenic medium for the isolation and differentiation of *Salmonella* spp., from clinical and non clinical specimens.

**2 - COMPOSITION -TYPICAL FORMULA \***

Peptones	10.0 g
Selective compounds	12.0 g
Cefsulodin	5.0 mg
Chromogenic mixture	0.9 g
Emulsifying agents	11.4 g
Opacifier	10.0 g
Agar	15.0 g
Purified water	1000 mL

\*The formula may be adjusted and/or supplemented to meet the required performances criteria.

**3 - PRINCIPLE OF THE METHOD AND EXPLANATION OF THE PROCEDURE**

*Salmonella* spp. remain one of the most important causes of foodborne gastroenteritis. Fluorogenic and chromogenic tests and media designed for the specific detection of *Salmonella* spp. have been available for at least 30 years. In 1987 a rapid fluorogenic screening reagent (MUCAP Test) for the identification of *Salmonella* colonies has been developed and proposed by Biolife Italiana, based on the detection of a specific *Salmonella* enzyme, C<sub>8</sub> esterase, by using a fluorogenic 4-methylumbelliferone-conjugated substrate.<sup>1</sup> Some years later, the same principle of detection of C<sub>8</sub> esterase enzyme has been exploited for the development of a chromogenic plating medium, Chromogenic Salmonella Agar, that demonstrated very high specificity and sensitivity for the detection of *Salmonella* spp.<sup>2,3</sup> Chromogenic Salmonella Agar is a selective and diagnostic medium useful for the isolation of *Salmonella* spp. from clinical and non clinical specimens and for the presumptive identification of the colonies. Chromogenic Salmonella Agar is included by ISTISAN Report<sup>4</sup> in the plating media range for the detection of *Salmonella* spp. and chromogenic media are included as the second plating medium in ISO Standards for detection of *Salmonella* in food and water.<sup>5,6</sup>

Peptones provide carbon, nitrogen, vitamins and trace elements for bacterial growth. The selective compounds incorporated in the medium are the following: cefsulodin, a third generation cephalosporin antibiotic that has very specific activity against *P. aeruginosa* and *S. aureus*, sodium desoxycholate that suppresses the growth of Gram-positive and some Gram-negative bacteria and Tergitol 4, active mainly against the growth of *Proteus* spp.

Differentiation of *Salmonella* from the other organisms that grow is achieved by:

- a chromogenic substrate for C<sub>8</sub> esterase enzyme, that is split by *Salmonella* spp. with the release of an insoluble magenta-red chromophore.
- a chromogenic glucopyranoside derivative which is split by β-glucosidase with the release of an insoluble blue-green chromophore.

Some *Enterobacteriaceae*, including *Klebsiella* and *Enterobacter*, but not *Salmonella*, are β-glucosidase positive and if growing will form blue-green or dark blue colonies, even if they are esterase positive, which make them easy to differentiate from magenta-red *Salmonella* colonies. The chromogenic and selective compounds of the medium also allow the detection of the rare lactose positive *Salmonella* strains, missed on traditional media based on lactose fermentation. Chromogenic Salmonella Agar is useful also for the detection of *S. Typhi* and *S. Paratyphi*. The ready-to-use plates include a compound that gives a white opaque background to the medium and enhances the colour of the colonies.

**4 - PHYSICAL CHARACTERISTICS**

Medium appearance	whitish opaque
Final pH at 20-25 °C	7.2 ± 0.2

**5 - MATERIALS PROVIDED - PACKAGING**

Product	Type	REF	Pack
Chromogenic Salmonella Agar	Ready-to-use plates	545350	2 x 10 plates ø 90 mm primary packaging: 2 cellophane sachets secondary packaging: cardboard box

**6 - MATERIALS REQUIRED BUT NOT PROVIDED**

Sterile loops and swabs, incubator and laboratory equipment as required, ancillary culture media and reagents for the identification of the colonies.

**7 - SPECIMENS**

Chromogenic Salmonella Agar is intended for the bacteriological processing of clinical specimens such as faeces and rectal swab. Good laboratory practices for collection, transport and storage of clinical specimens should be applied.<sup>7</sup> Consult appropriate standard methods for details of collection and preparation of non-clinical specimens.<sup>5,6</sup>



## 8 - TEST PROCEDURE

Allow plates to come to room temperature and to dry the surface of the medium. Inoculate and streak the specimen with a loop over the four quadrants of the plate to obtain well isolated colonies, ensuring that sections 1 and 4 do not overlap. Alternatively, if the material is being cultured directly from a swab, roll the swab over a small area of the surface at the edge; then streak from this inoculated area.

Maximal recovery of *Salmonella* from faecal specimens is obtained by using the enrichment step in Selenite Broth followed by subculture to Chromogenic Salmonella Agar and to a second plating medium.

Incubate inoculated plates with the specimen or with specimen enriched in liquid medium, in aerobic conditions at 35-37°C for 18-24 hours.

Consult appropriate references for the detection of *Salmonella* in foods and water.<sup>5,6</sup>

## 9 - READING AND INTERPRETATION

After incubation, observe the bacterial growth and record the specific morphological and chromatic characteristics of isolated colonies. Interpretation of colonies colours:

Microorganism	Growth characteristics
<i>Salmonella</i> spp.	good growth, magenta-red colonies
<i>Salmonella</i> spp. lac+	good growth, magenta-red colonies
<i>Salmonella</i> Typhi	good growth, magenta-red colonies
<i>E.coli</i>	poor growth with colourless colonies
<i>Enterobacter</i> spp.	growth with blue-green colonies
<i>Klebsiella</i> spp.	poor growth with blue-green colonies
<i>Pseudomonas</i> spp.	inhibited
<i>Proteus</i> spp.	poor growth with pale brown or green colonies
Gram-positive bacteria	inhibited

## 10 - USER QUALITY CONTROL

All manufactured lots of the product are released for sale after the Quality Control has been performed to check the compliance with the specifications. However it is responsibility of the end-user to perform Quality Control testing in accordance with the local applicable regulations, in compliance with accreditation requirements and the experience of the Laboratory. Here below are listed some test strains useful for the quality control.

CONTROL STRAINS	INCUBATION T° / T / ATM	EXPECTED RESULTS
S.Typhimurium ATCC 14028	35-37°C / 18-24h / A	growth, magenta-red colonies
S. Enteritidis ATCC 13076	35-37°C / 18-24h / A	growth, magenta-red colonies
<i>E. aerogenes</i> ATCC 13048	35-37°C / 18-24h / A	growth, blue-green colonies
<i>P. aeruginosa</i> ATCC 27853	35-37°C / 18-24h / A	inhibited

A: aerobic incubation; ATCC is a trademark of American Type Culture Collection

## 11 - PERFORMANCES CHARACTERISTICS

Chromogenic Salmonella Agar was evaluated by Babic-Ergeg et al.<sup>2</sup> on 3,000 stool specimens, 45 of which positive for *Salmonella*, including SS Agar as the reference medium. The authors reported a sensitivity of 100% and a specificity of 99% in the isolation and preliminary identification of *Salmonella* colonies.

In another independent study<sup>3</sup>, 50 pure cultures of *Salmonella* of clinical origin, gave all the specific chromatic reactions; among the other 80 strains of Gram negative bacteria tested, not belonging to the *Salmonella* genus, 3 out of 3 strains of *P.aeruginosa* and 1 out of 3 strain of *A.baumannii* provided chromatic results similar to *Salmonella* spp. (red-pink colonies), the remaining 76 strains of *Enterobacteriaceae* gave non-typical chromatic reactions; 20 out of 20 strains of Gram positive bacteria were totally inhibited.

Chromogenic Salmonella Agar performance was evaluated with an in-house study, compared to Hektoen Enteric Agar (HEA). Productivity, selectivity and specificity have been evaluated by semi-quantitative ecometric technique, incubating at 35-37°C for 18-24 hours, using 43 bacterial strains: 8 target strains and 35 non target strains. 8 *Salmonella* strains, including 2 *S.Typhi*, showed a good growth with magenta-red colonies; 3 *Shigella* strains showed a poorer growth than on HEA with colourless colonies; 22 *Enterobacteriaceae* strains belonging to 9 genera showed a poorer growth than on HEA with colourless or blue-green colonies; 4 *P.aeruginosa* strains were totally inhibited; 2 non fermenters strains were totally inhibited and *A.hydrophila* grew with magenta red colonies; 1 Gram positive strain was totally inhibited and 1 yeast strain was partially inhibited showing colourless colonies.

Prior to release for sale a representative sample of all lots of ready-to-use plates of Chromogenic Salmonella Agar and of the raw materials used for the production of prepared plates (dehydrated Chromogenic Salmonella Agar REF 405350 supplemented with Salmonella Selective Supplement REF 4240013) are tested for productivity specificity and selectivity by comparing the results with a previously approved Reference Batch.

Productivity is tested by a quantitative test with the target strains S.Enteritidis ATCC 13076 and S.Typhimurium ATCC 14028; Chromogenic Salmonella Agar plates are inoculated with decimal dilutions in saline of a suspension of colonies and incubated at 35-37°C for 18-24 hours. The colonies are enumerated on Test Batch (TB) and Reference Batch (RB) and the productivity ratio ( $Pr = \text{UFC}_{\text{TB}} / \text{UFC}_{\text{RB}}$ ) is calculated. If  $Pr$  is  $\geq 0,7$  and if the colonies' colour is typical (magenta red colonies) the results are considered acceptable and conform to the specifications.

Specificity is evaluated with by semi-quantitative ecometric technique with the following non-target strains: *S.flexneri* ATCC 12022, *E.aerogenes* ATCC 13048, *E.coli* ATCC 8739; *E.aerogenes* grows with blue-green colonies, the growth of *S.flexneri* is not inhibited and the colonies are colourless, *E.coli* is partially inhibited with colourless colonies. Selectivity is evaluated with modified Miles-Misra surface drop method by inoculating the plates with decimal dilutions in saline from  $10^{-1}$  to  $10^{-4}$  of a 0.5 McFarland suspension of the non-target strains *P.vulgaris* ATCC 13315, *A.calcoaceticus* ATCC 19606, *P.aeruginosa* ATCC 27853, *A.hydrophila* ATCC 7965, *E.faecalis* ATCC 19433, *Mucor* CBM1. *A.hydrophila* is partially inhibited and grows with magenta colonies; the growth of other non-target strains is totally inhibited at the dilution  $10^{-1}$ .

## 12 - LIMITATIONS OF THE METHOD



- A single medium is only rarely useful to recover all pathogens contained in a specimen. Therefore, additional media for the isolation of *Salmonella*, with lower selectivity such as Mac Conkey Agar should be used; other media for the isolation of other enteric pathogens must be inoculated with the specimen.
- Some strains of *Pseudomonas*, *Acinetobacter* and *Aeromonas*, resistant to antimicrobial agents of the medium, may grow with red-pink colonies, differentiable from *Salmonella* with oxidase test.
- The growth rate on the plates also depends on the nutritional requirements of *Salmonella*. It is possible that some strains with particular metabolic characteristics may not grow on the medium or grow colourless (e.g. *Salmonella enterica* serovar Dublin grows with white colonies).
- Even if the microbial colonies on the plates are differentiated on the basis of their morphological and chromatic characteristics, it is recommended that biochemical, immunological, molecular, or mass spectrometry testing be performed on isolates, from pure culture, for complete identification. If relevant, perform antimicrobial susceptibility testing.
- This culture medium is intended as an aid in the diagnosis of infectious disease; the interpretation of the results must be made considering the patient's clinical history, the origin of the sample and the results of other diagnostic tests.

**13 - PRECAUTIONS AND WARNINGS**

- This product is a qualitative *in vitro* diagnostic, for professional use only; it is to be used by adequately trained and qualified laboratory personnel, observing approved biohazard precautions and aseptic techniques.
- This product is not classified as dangerous according to current European legislation.
- This culture medium contains raw materials of animal origin. The *ante* and *post mortem* controls of the animals and those during the production and distribution cycle of the raw materials, cannot completely guarantee that these products do not contain any transmissible pathogen. Therefore, it is recommended that the ready-to-use plates be treated as potentially infectious, and handled observing the usual specific precautions: do not ingest, inhale, or allow to come into contact with skin, eyes, mucous membranes. Download the TSE Statement from the website [www.biolifeitaliana.it](http://www.biolifeitaliana.it), describing the measures implemented by Biolife Italiana for the risk reduction linked to infectious animal diseases.
- All laboratory specimens should be considered infectious.
- The laboratory area must be controlled to avoid contaminants such as culture medium or microbial agents.
- Each plate of this culture medium is for single use only.
- Ready-to-use plates are not to be considered a "sterile product" as they are not subject to terminal sterilization but a product with controlled bio contamination, within the limits of defined specifications reported on the Quality Control Certificate.
- Sterilize all biohazard waste before disposal. Dispose the unused medium and the plates inoculated with samples or microbial strains in accordance with current local legislation.
- The Certificates of Analysis and the Safety Data Sheet are available on the website [www.biolifeitaliana.it](http://www.biolifeitaliana.it).
- The information provided in this document has been defined to the best of our knowledge and ability and represents a guideline for the proper use of the product but without obligation or liability. In all cases existing local laws, regulations and standard procedures must be observed for the examination of samples collected from human and animal organic districts, for environmental samples and for products intended for human or animal consumption. Our information does not relieve our customers from their responsibility for checking the suitability of our product for the intended purpose.

**14 - STORAGE CONDITIONS AND SHELF LIFE**

Upon receipt, store plates in their original pack at 2-8°C away from direct light. If properly stored, the plates may be used up to the expiration date. Do not use the plates beyond this date. Plates from opened plastic sachet can be used for 7 days when stored in a clean area at 2-8°C. Do not use the plates if the plastic sachet is damaged or if the dish is broken. Do not use the plates with signs of deterioration (e.g. microbial contamination, dehydration, shrinking or cracking of the medium, atypical colour, excess of moisture).

**15 - REFERENCES**

1. Pontello M, Russolo S, Carozzi F, Bottirol U. Evaluation of a new rapid method (MUCAP Test) for the presumptive identification of Salmonella on primary isolation media. 5th Int. Simp. on Rapid Method and Aut. in Microb. and Immunol. Florence 4-6 nov. 1987
2. Babic-Erceg A et al. 12th European Congress of Clinical Microbiology and Infectious Diseases. Milan, April 24-27, 2002
3. Andreoni S. et al. Microbiologia Medica, 2002.
4. Istituto Superiore di Sanità Le infezioni da Salmonella: diagnostica, epidemiologia e sorveglianza. Caterina Graziani, Pasquale Galetta, Luca Busani, Anna Maria Dionisi, Emma Filetici, Antonia Ricci, Alfredo Caprioli, Ida Luzzi 2005, 49 p. Rapporti ISTISAN 05/27
5. ISO 6579-1:2017 Microbiology of the food chain — Horizontal method for the detection, enumeration and serotyping of Salmonella.
6. ISO 19250:2010 Water quality — Determination of Salmonella species
7. Baron EJ, Specimen Collection, Transport and Processing: Bacteriology. In Jorgensen JH, Carrol KC, Funke G et al. editors. Manual of clinical microbiology, 11th ed. Washington, DC: American Society for Microbiology; 2015. p.270

**TABLE OF APPLICABLE SYMBOLS**

<b>REF</b> or <b>REF</b> Catalogue number	<b>LOT</b> Batch code	<b>IVD</b> <i>In vitro</i> Diagnostic Medical Device	Manufacturer	Use by
Temperature limitation	Contents sufficient for <n> tests	Consult Instructions for Use	For single use only	Fragile, handle with care

**REVISION HISTORY**

Version	Description of changes	Date
Instructions for Use (IFU) - Revision 2	Updated layout and content in compliance with IVDR 2017/746	2020/05
Instructions for Use (IFU) - Revision 3	Removal of obsolete classification	2023/03

Note: minor typographical, grammatical, and formatting changes are not included in the revision history.